PREAMP/AMP/DISC
MODEL 813

INSTRUCTION MANUAL

November, 1969

Canberra Industries
45 Gracey Ave.
Meriden, Connecticut 06450

Telephone: 203-238-2351

PREAMP/AMP/DISC

MODEL 813

CONTENTS

Page

1 INTRODUCTION 1-1

2 SPECIFICATIONS

2.1 Preamp and Amplifier 2-1
2.2 Discriminator 2-1
2.3 Connectors 2-1
2.4 Power 2-2
2.5 Physical 2-2

3 CONTROLS AND CONNECTORS

3.1 General 3-1
3.2 Controls 3-1
3.3 Connectors 3-1

4 OPERATING INSTRUCTIONS

4.1 General 4-1
4.2 Set Up 4-1
4.3 Checkout Procedure 4-1

5 THEORY OF OPERATION

5.1 General 5-1
5.2 Preamplifier 5-1
5.3 First Amplifier 5-1
5.4 Second Amplifier 5-1
5.5 Third Amplifier 5-2
5.6 Output Amplifier 5-2
5.7 Discriminator 5-2
5.8 Reference Voltage Generator 5-2
5.9 Output Monostable 5-2
5.10 Output Drivers 5-2

SECTION 1
INTRODUCTION

The Canberra Model 813 contains a charge sensitive FET input preamplifier, a linear amplifier with a maximum gain of 600 and an integral discriminator. It accepts the negative or positive charge output of gas proportional counters or semiconductor detectors and provides, at the AMP OUT connector, a near Gaussian bipolar voltage pulse. The charge sensitive input enables the use of relatively long connecting cables without signal distortion.

Amplifier gain is established by front panel controls; a five position switch provides a 16:1 range in 2:1 steps; a front panel single-turn continuous control provides a 3:1 range.

The module can accept either a positive or negative input signal by use of a front panel polarity selection switch. An integral discriminator provides a positive 8 volt rectangular pulse at the DISC OUT connector for each amplifier output which exceeds a selected threshold. Discriminator Threshold is selected by a ten turn front panel control and spans a range from 50 millivolts to 10 volts. The Model 813 can be used with all Canberra 800 and 1400 Series modules.

SECTION 2

SPECIFICATIONS

2.1 PREAMP AND AMPLIFIER

INPUTS	Front panel BNC connectors accept negative or positive charge signals from gas proportional counters or semiconductor detectors; input sensitivity, 2V/picocoulomb
GAIN STABILITY	0.01%/°C
GAIN CONTROLS	COARSE: 16:1 range in binary steps FINE: 3:1 continuous range
PULSE SHAPING	1.25 microsecond time constant, near-Gaussian bipolar
AMP OUTPUT	Saturation Levels: ±10.0 volts Integral Linearity: Better than 0.5% from 0.05 to 10 volts Impedance: Less than 1 ohm Output Connector: Front panel BNC
NOISE PERFORMANCE	2.9 keV + 0.07 keV/pf detector capacitance (FWHM, Ge detector)

2.2 DISCRIMINATOR

SENSITIVITY	50 millivolts to 10 volts, selected by front panel ten-turn potentiometer
LINEARITY	±0.5%, 50 millivolts to 10 volts
STABILITY	5mV/°C
OUTPUT	Front panel BNC connector
IMPEDANCE	10 ohms
PULSE SHAPE	Duration: 1 microsecond square pulse Rise Time: 50 nanoseconds Polarity: Positive. Amplitude: 8 volts

2.3 CONNECTORS

INPUT	BNC UG/1094-U
OUTPUTS	BNC UG/1094-U

2.4 POWER

+24V	50mA	–	+12V	50mA
-24 V	60mA	–	- 12V	55mA

2.5 PHYSICAL

SIZE — Standard single-width module (1.35 inches wide) per TID-20893

WEIGHT — 1.4 lb.

SECTION 3

CONTROLS AND CONNECTORS

3.1 GENERAL

This section describes the functions of the controls and connectors located on the module. It is recommended that this section be read before proceeding with the operation of the module.

3.2 CONTROLS

3.2.1 COARSE GAIN CONTROL

Front panel rotary switch selects the factor by which the signal at the PREAMP IN (or AMP IN, depending on the switch position) is to be amplified. Gain positions are 4, 8, 16, 32, and 64.

3.2.2 FINE GAIN

Front panel single-turn potentiometer which permits a range of 3:1 of the output selected by the COARSE GAIN control.

3.2.3 DISCRIMINATOR CONTROL

This front panel ten-turn control is used to select a threshold level for the AMP OUTPUT above which a positive eight volt, one microsecond rectangular pulse will be generated at the DISC OUTPUT connector. This control can be adjusted for sensitivities from 50 millivolts to ten volts.

3.2.4 AMP POS/NEG SWITCH

Front panel two-position toggle switch used to set the polarity which will be accepted at the AMP or PREAMP input.

3.2.5 PREAMP IN/OUT SWITCH

Front panel two-position toggle switch used to connect or disconnect the preamplifier from the amplifier.

3.3 CONNECTORS

3.3.1 DISC OUT CONNECTOR

Provides a positive eight volt, one microsecond pulse each time the amplifier output exceeds the discriminator threshold setting.

3.3.1 AMP IN CONNECTOR

Accepts negative or positive tail pulses from a preamplifier.

3.3.2 AMP OUT CONNECTOR

Provides a positive-lobe leading, near-Gaussian pulse of up to ten volts. The amplitude is adjustable by the COARSE and FINE GAIN controls. The output impedance is less than one ohm.

3.3.3 TEST IN CONNECTOR

This input is used to check the charge sensitivity and noise calibration of the module. The nominal test capacitance value is 1pf. A Canberra Model 1407 Pulser can be used to supply the test pulse. Refer to Section 4 for further details.

SECTION 4

OPERATING INSTRUCTIONS

4.1 GENERAL

The purpose of this section is to familiarize the user with the controls of the Model 813 Preamp/Amp/Disc and to check that the unit is operating correctly. Since it is difficult to determine the exact system configuration in which the module will be used, explicit operating instructions cannot be given. However, if the following procedures are carried out, the user will gain sufficient familiarity with this instrument to permit its proper use in the system at hand.

4.2 SET UP

1. Insert the Model 813 PAD module in an AEC compatible bin such as the Canberra Model 800 or 1400.

2. Connect the positive output from a tail pulse generator to the TEST IN connector of the Model 813 PAD.

3. Set the AMP POS/NEG switch at NEG since the preamplifier inverts the signal to the amplifier stage.

4. Set the PREAMP IN/OUT switch at IN.

5. Connect an oscilloscope to the AMP OUTPUT. Set the oscilloscope sensitivity at 5V/cm and 2 microseconds/cm. Terminate the output with a 100 ohm load.

6. Set the COARSE GAIN control at 64.

7. Set the FINE GAIN control at 10.

4.3 CHECKOUT PROCEDURE

4.3.1 INITIAL CHECKOUT

1. Having performed the operations in Section 4.2, increase the pulser output and note that the waveform is as shown in Figure 1.

2. Set the COARSE GAIN control at 32. Observe that the output is attenuated by a factor of 2. Rotate the FINE GAIN control and note that the output ranges from about 5 volts to about 1.6 volts, a nominal 3:1 range.

3. Switch the COARSE GAIN CONTROL to 4, 8, 16, and 64, noting that the output increases by factors of 2. Rotate the FINE GAIN control at each setting of the COARSE GAIN control and note that the output is variable from 1/3 maximum to full maximum at each COARSE GAIN setting.

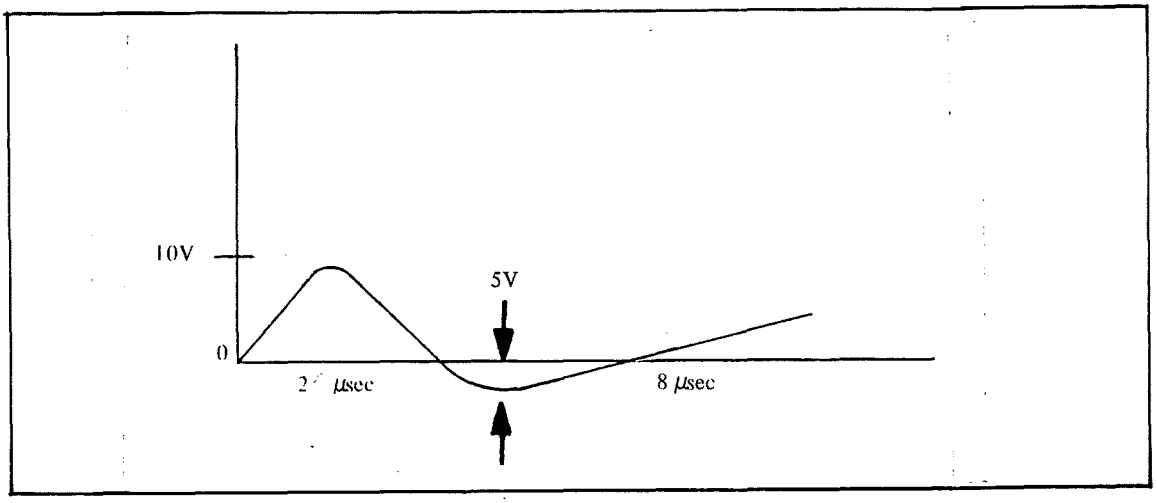

Figure 1. AMP OUTPUT Waveform.

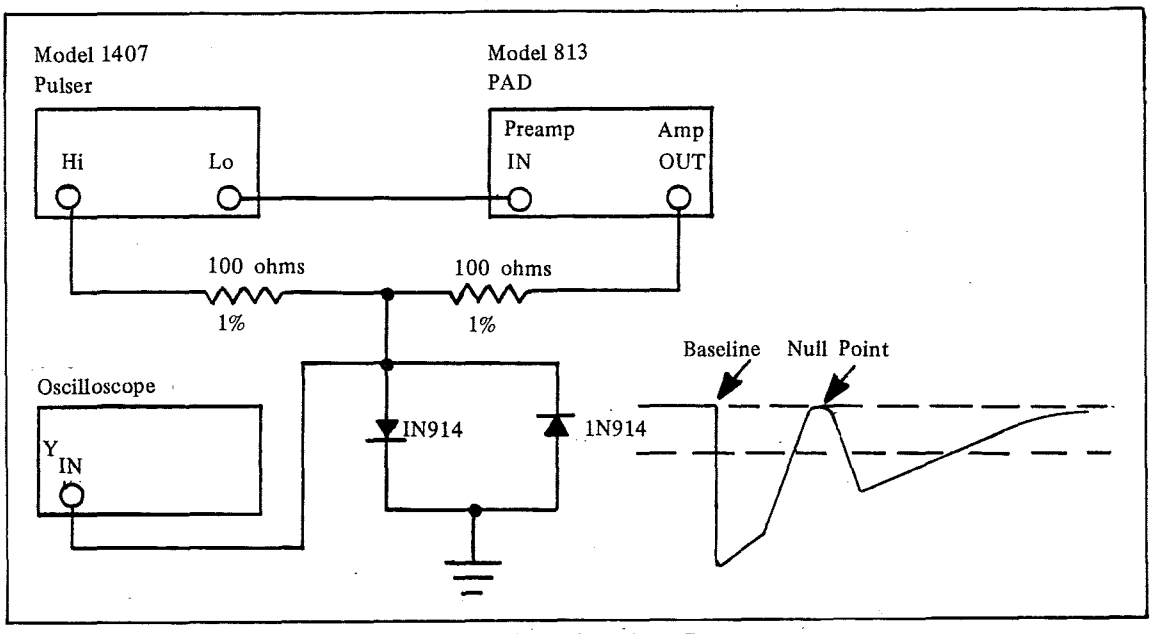

Figure 2. Linearity Test Setup.

4. Set the gain controls at their maximum settings. The overall gain of the Amplifier is approximately 600. Observe an output of approximately ten volts for a 7-9 millivolt input to the preamplifier.

4.3.2 LINEARITY TEST

1. Set up the system as shown in Figure 2.

2. This test is performed by adjusting the pulser attentuators and amplifier gain so that with a ten volt high level (Direct) output from the pulser, the output from the amplifier is also exactly ten volts. This may be ascertained by adjusting the pulser attenuators and amplifier gain so that the null point observed on the oscilloscope (using the highest vertical gain) is at exactly the same level as the baseline.

3. When the condition described in step 2 is obtained, rotate the pulser pulse height control slowly to the lowest level that will still trigger the oscilloscope; observe the maximum difference between the baseline and the null point. The integral linearity of the amplifier is then equal to

$$\frac{\text{(Maximum deviation in volts) x2 x100\%}}{\text{10 volts}}$$

The maximum deviation must thus be less than 25mV in order to meet the 0.5% specification. The additional factor of two is added to compensate for the voltage division performed by the test circuitry.

4.3.3 DISCRIMINATOR CHECK

1. Connect an oscilloscope to the DISC OUT connector (5V/cm, 1 microsecond/cm).

2. Set the DISC control at 8.0

3. Connect the positive output of the pulser to the TEST IN connector.

4. Set the AMP POS/NEG switch at NEG since the preamplifier inverts the signal to the amplifier..

5. Set the PREAMP IN/OUT switch at IN.

6. Increase the pulse height of the pulser until an output just appears at the DISC OUT connector. The AMP OUT pulse should be 8.0 ±0.1 volts. The DISC OUT signal should be a positive eight volt pulse with a maximum rise time of 50 nanoseconds, and a pulse width of one microsecond.

NOTE

If it is desired to change the width of the discriminator output, adjust RV-10, located on the printed circuit card, to the value desired. The adjustment range is approximately 0.5 microsecond to 2.5 microseconds.

7. Set the DISC control at other positions and note that the DISC OUT signal appears when the AMP OUT voltage is the same as that indicated on the DISC control.

4.3.4 CONNECTION TO A DETECTOR

1. The Model 813 PAD may be used with a gas proportional counter, a silicon surface barrier detector, or a lithium drifted germanium or silicon detector.

2. Apply the bias to the detector as shown in Figure 3. The bias resistor should typically be between one and 100 Megohms. As the detector leakage current increases, the bias resistance must be decreased. The resistor is selected so that the voltage drop across it is approximately 100-200 volts or less, if possible. To reduce hum and noise pickup, shield the bias resistor, all connecting cables, and the connections to the bias supply, detector, and Model 813 with coaxial cable or metal shielding.

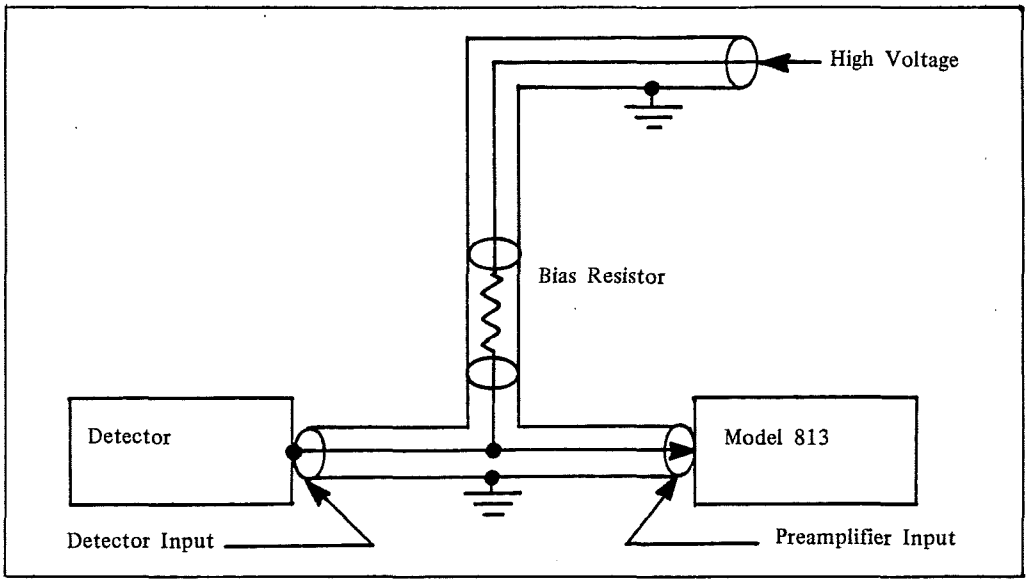

Figure 3. Typical Detector Interconnections.

SECTION 5

THEORY OF OPERATION

5.1 GENERAL

The circuitry for the following descriptions can be found on schematic drawing D-11904.

5.2 PREAMPLIFIER

The preamplifier in the Model 813 converts charge impulses from a solid state detector to a voltage pulse (a tail pulse). The charge sensitivity is determined by feedback capacitor C3. The detector signal output goes to Q25, an FET which exhibits a high input impedance and a low noise level. The signal is amplified by the common base stage Q26. Q1 and Q2, which are in a Darlington configuration, provide a low output impedance for the preamplifier output.

5.3 FIRST AMPLIFIER

The tail pulse output of the preamplifier goes through C11 to the PREAMP switch (S3), which switches the preamplifier in or out of the circuit. The output of S3 is connected to the AMP POS/NEG switch (S1). If the preamp is not used, a signal may be fed to the AMP IN BNC which is also connected to the PREAMP switch. The first amplifier is made up of Q3, Q4, and Q5. This amplifier circuitry has a gain of 4.22. DC balance, for a positive input, is achieved by RV-1 which adjusts the current through Q3. Negative input is achieved by adjusting the bias by use of RV-2. Q3 is basically an impedance matching stage. Q4 is a gain stage. It is followed by Q5 which is an emitter follower for impedance matching of the first amplifier output (TP-3).

The Model 813 preamplifier shaping occurs at the input to the amplifier by use of a differentiation network (C11 and the input resistance of the first amplifier) for positive polarity. This network has a time constant of 50μsec. The first amplifier is followed by another differentiation network (C23 and R28 in parallel with the input resistors R29, 30, and 31 of the second amplifier). These components form the pole-zero compensation network. It has a time constant of 1.22μsec. Pole-zero is adjusted by RV-3.

5.4 SECOND AMPLIFIER

The pole-zero network goes to the second amplifier through the COARSE GAIN switch (S2a). The second amplifier consists of an input impedance stage (Q6), a gain stage (Q7), and an output impedance stage (Q8). The DC balance of the second amplifier is adjusted by RV-4 which varies the current through Q6. The second amplifier has a maximum gain of 3.8

The overall gain of the PAD is controlled by the gain of the second amplifier in addition to the input/output amplitudes. The gain of the second amplifier is controlled by the front panel FINE GAIN control (RV-5) which varies the second amplifier gain from 2.6 to 8.4. The COARSE GAIN switch (S2a), along with R29, R30, and R31, controls the input amplitude. S2b and R32-38 control the output amplitude to TP-2 (third amplifier input).

5.5 THIRD AMPLIFIER

The third amplifier is an integrating amplifier composed of an I.C. operational amplifier (A1) and integrating networks (R57, R58, R55, C37, C39, and C33). This amplifier has a gain of approximately 6. The output of the third amplifier (TP-4) goes to a final differentiation network (C40 and R64) which is also the input to the final amplifier.

5.6 OUTPUT AMPLIFIER

The output amplifier consists of Q9 and Q10, which form an emitter coupled input stage, a gain stage (Q11), and complementary emitter followers (Q12 and Q13). In this way a low output impedance for the AMP OUT BNC and the DISC input can be obtained. DC balance is obtained by RV-6 which is used to adjust the bias of Q9 and Q10. The final amplifier has a gain of 7.8 and can produce a 10 volt output into 93Ω.

5.7 DISCRIMINATOR

The output amplifier goes to the discriminator section of the Model 813. The discriminator consists of four basic sections: an I.C. discriminator, a reference voltage generator, an output monostable, and an output driver.

The I.C. discriminator is a μA710 voltage comparator (A2) which yields a positive pulse when the positive input (pin 2) is more positive than the negative input (pin 3). The positive input of the μA710 is driven by the amplifier output signal via Q17.

Q17 is an emitter follower which prevents the input impedance of the μA710 from loading down the amplifier section. R89 and R90 divide the input signal by 0.4. The negative input of the μA710 goes through Q18 from the reference voltage generator. Q18 is an emitter follower and prevents loading of the reference voltage generator by the negative input.

5.8 REFERENCE VOLTAGE GENERATOR

The reference voltage generator provides the voltage to which the input signal is compared by the μA710. This voltage is developed by R80, RV-7, and the front panel DISC potentiometer (RV-8) in series across +12 volts. The voltage on the wiper of RV-8 is fed through two emitter followers (Q14 and Q15), one NPN and the other PNP. Therefore, the voltage at the emitter of Q15 is the same as the voltage at the RV-8 wiper. Q16 is a constant current source for keeping the voltage drop across RV-9 constant. RV-9 is used to calibrate RV-8 at the low end while RV-7 calibrates the high end of RV-8.

5.9 OUTPUT MONOSTABLE

The output of A2 goes to the output monostable which is made up of Q19 through Q22. Q20 and 21 are used to speed up the switching time of the monostable so that the rise and fall times are fast. RV-10 adjusts the length of the monostable output pulse from 0.5 to 2.5μsec.

5.10 OUTPUT DRIVERS

The output monostable is followed by output drivers (Q23 and 24). These drivers provide a very low output impedance and prevent any output load from ruining the fast rise and fall times of the discriminator output.

This manual is applicable to the module whose Serial Number is_____